



Result Receival Dates

	JUNE
Lab Code	
J	04-Jun-08
M	06-Jun-08
I	12-Jun-08
F	17-Jun-08
K	17-Jun-08
A	18-Jun-08
E	24-Jun-08
L	24-Jun-08
O	25-Jun-08
H	27-Jun-08
B	30-Jun-08
G	30-Jun-08
C	NOT RECEIVED
D	NOT RECEIVED
N	NOT RECEIVED

**Just a reminder to get results in promptly*

Discussion of Results

Test Weight

Results received this round were fairly good with no labs straying too far from the mean. The lowest result was from lab M with a mean difference of -0.88. Lab F submitted the highest with a mean difference of 0.82.

Impurities

Lab B produced a significantly high result this round with a mean difference of 1.20 compared to 0.22 in the previous round. Lab G submitted the lowest result with a mean difference of -0.87. Lab G also submitted the lowest result in the previous round recording -0.39.

Oil Rapid

Lab O performed better this round with a mean difference of -0.67 compared to -1.19 in the previous round. Lab M continues to submit the closest to the mean recording -0.03 this round.



07/08 AOF Test Check Program Monthly Report

Round 7

JUNE 2008

2/6/2008 – 30/6/2008

Oil Solvent

Again, labs E, F and G submitted significantly far from the mean submitting differences over +/-1.00%. Lab B also submitted a high result recording 0.94. Note that significant differences separate Oil Solvent and Oil Rapid results for labs F and G.

Oil Solvent (AOCS Method Am 2-93)

Good results were received from the three participating labs.

Oil SFE

Only lab J submitted results for Oil SFE this round.

Moisture Oven

Lab F produced an outlier recording -0.88 this round and was omitted from the mean and standard deviation. Excellent results were achieved by the remaining participants.

Moisture Rapid

Results were similar to that seen in the previous round with reasonably good results overall.

Oleic Oil

Labs B and O produced outliers this round recording -1.05 and 0.96.

Linoleic Oil


Good results were generated this round with all labs submitting relatively close to the mean.

Free Fatty Acid

Good results were also submitted for FFA to produce a low standard deviation of 0.23.

AOF Test Check Program JUNE 2007/2008
Sample Number 7 Summary

Lab Code	Oil Rapid % (Clean)	Oil Solvent % (Clean)	Oil Solvent % (Clean) AOCS	Oil % SFE (Clean)
A	41.09			
B	40.63	40.29	40.07	
C				
D				
E	40.65	40.71		
F	39.40	38.01		
G	40.22	37.72	39.04	
H	39.25		39.65	
I	40.20	39.14		
J	40.83			38.65
K	39.55	39.56		
L		39.90		
M	40.09			
N				
O	39.45	39.40		
Mean	40.12	39.34	39.58	38.65

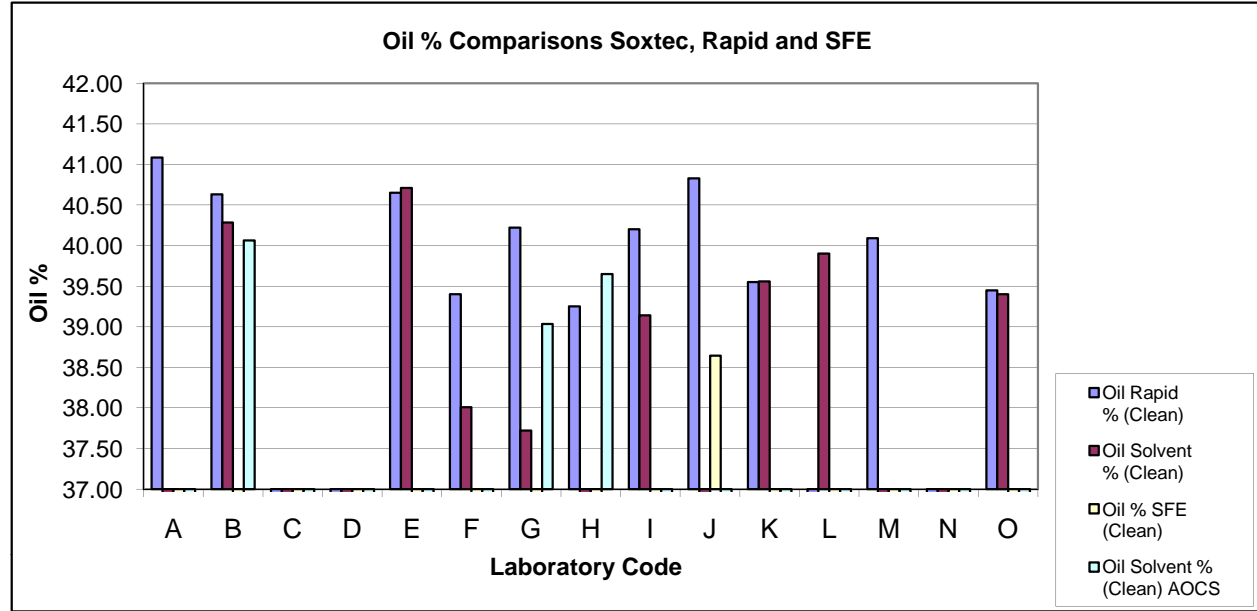

Lab Code	Moisture % Oven Result	Moisture % Rapid Result
A		4.96
B	5.43	5.69
C		
D		
E	5.81	5.90
F	4.62	5.30
G	5.36	
H	5.70	5.65
I	5.63	5.45
J	5.45	5.37
K	5.30	5.05
L	5.56	
M	5.46	5.05
N		
O	5.30	
Mean	5.50	5.38

